

# Effects of Tubing Changes on Calibration of SONOFLOW® Ultrasonic Sensors



TECHNICAL NOTE



**SONOFLOW® CO.55 Flow Sensors** are factory calibrated to customer specific tubing to ensure the most accurate and reliable measurement results. The unique properties of the tubing, such as material of composition, inner diameter, and durometer affect the speed at which the ultrasound travels through the tubing and are accounted for during the calibration process. If CO.55 sensors are used with a tubing that differs from the tubing used for calibration, there will be a shift in the calibration causing potential inaccuracies in reported measurement. Tubing changes can be accounted for with adjustents using SONOFLOW® software or through factory recalibration. While SONOFLOW® CO.55 sensors can be accurately calibrated for most industry standard tubing, it is important to understand how tubing changes can affect the calibration and therefore the reported flow measurement.

## Flow Sensor Set-Up for Comparison of Multiple Tubing Types


Sensor	SONOFLOW® CO.55/080 V2.0 Sensor
Tubing Size	1/4" ID x 3/8" OD
Baseline Calibration	Standard factory calibration for Masterflex® PCS [water, 23°C ±2 K, standard sensor flow range]
Comparison	Made by changing tubing while all other parameters remain constant



## Calibration Shift Due to Tubing Change

The Diagram shows the comparison of multiple tubing types used on the SONOFLOW® sensor calibrated for Masterflex® PCS

**Conclusion:** Changing tubing will cause a calibration shift. Sensor must be adjusted properly for the specific tubing type being used.

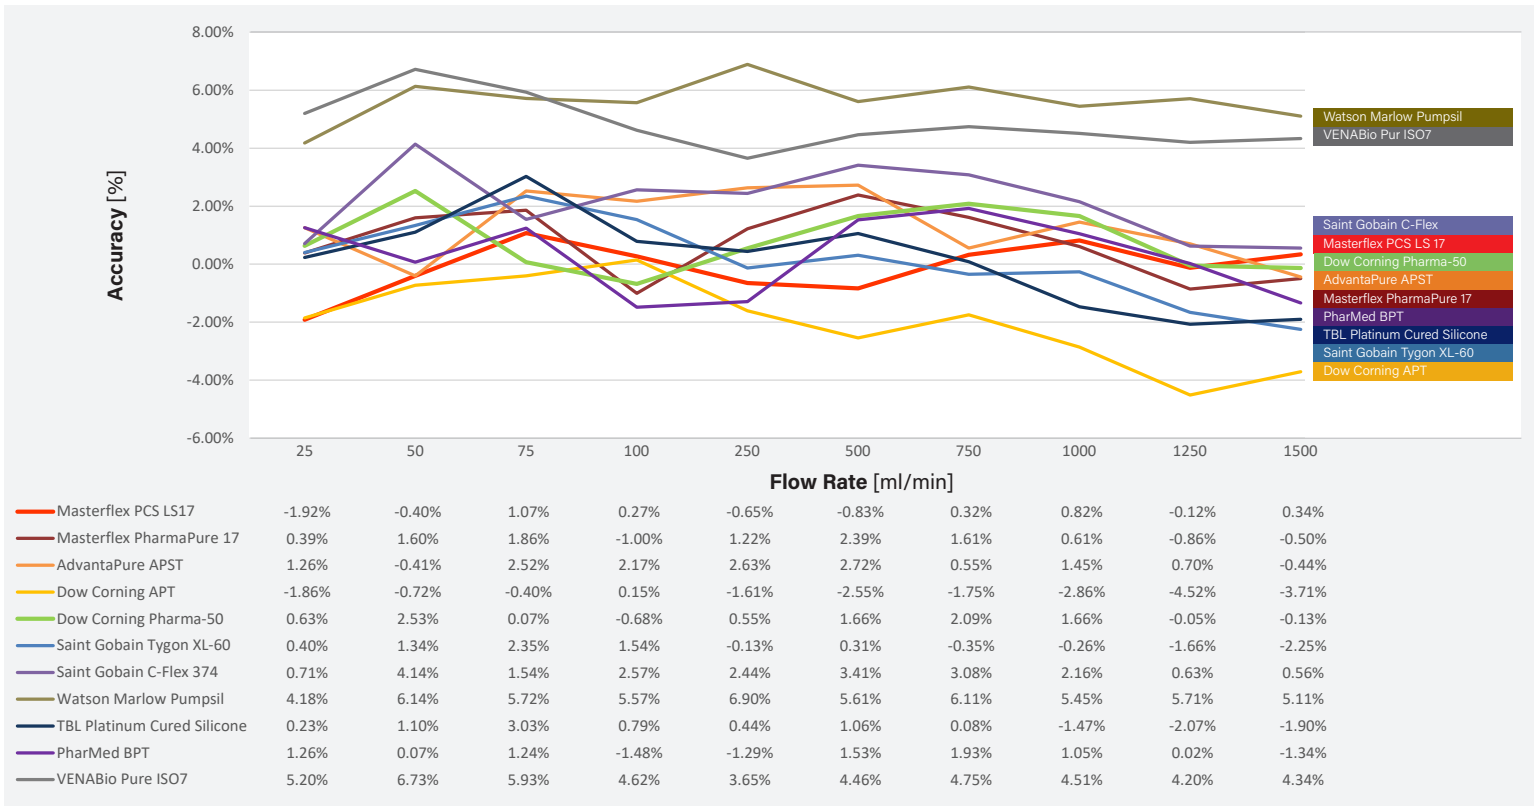




## Tube Comparison Test 2: Same Material, Different Manufacturer

Manufacturers have specific proprietary formulations for tubing materials which may alter the ultrasonic transmission. Two platinum cured silicone tubes from different manufacturers may perform differently in an ultrasonic sensor.

Using Masterflex® PCS as a baseline, the diagram at the right shows the shift when changing from one PCS to another from a different manufacturer.

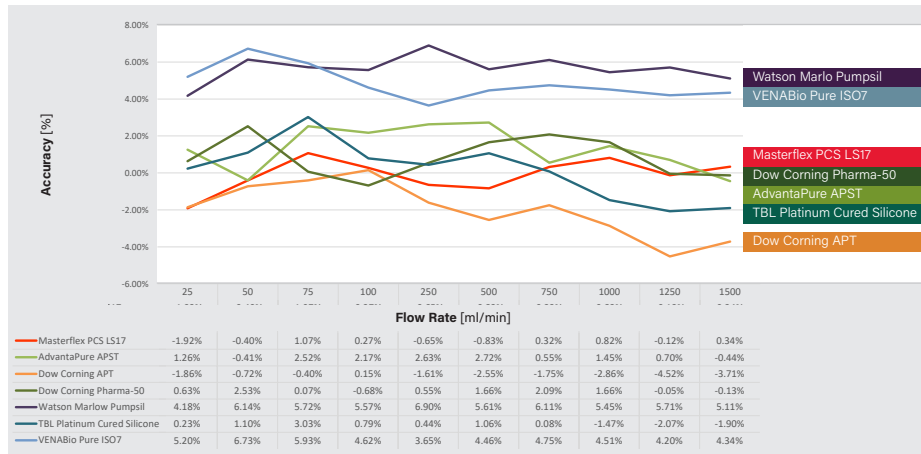


**CONCLUSION:** Not all silicone is the same. The sensor must be adjusted if changing from one manufacturer's silicone tubing to another.

## Tube Comparison Test 3: Different Inner Diameter (ID)

Inner diameter of the tubing affects the cross sectional area inside the tube, which is a contributing factor in the flow measurement calculation.

Diagrams at the right show how tubing from the same manufacturer with the same composition will differ in measurement calculation when the ID of the tubing is not the same.

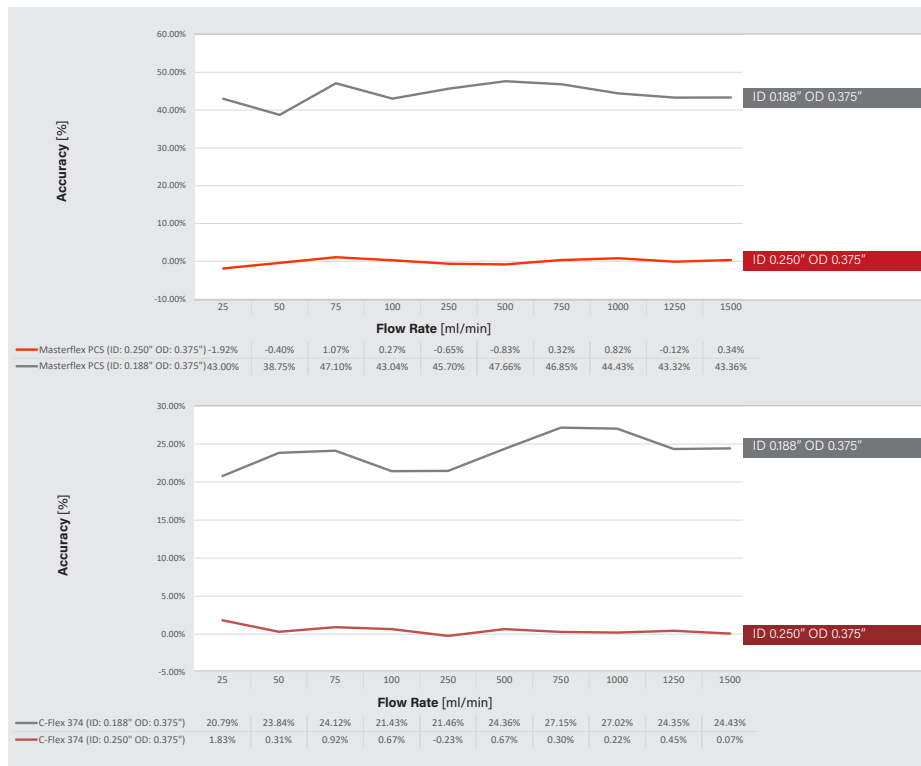


**CONCLUSION:** The sensor must be adjusted when changing to a tubing with the same OD but different ID.

## Tubing Comparison Test 4: Different Durometer

Durometer of the tubing will also affect the calibration because the ultrasound will travel at different speeds depending on durometer. In addition, tubes with differing durometers fit differently in the sensor, affecting the inner diameter measurement and area.

The diagram at the right shows a sensor calibrated on Dow Corning Pharma 50 compared to Pharma 80.

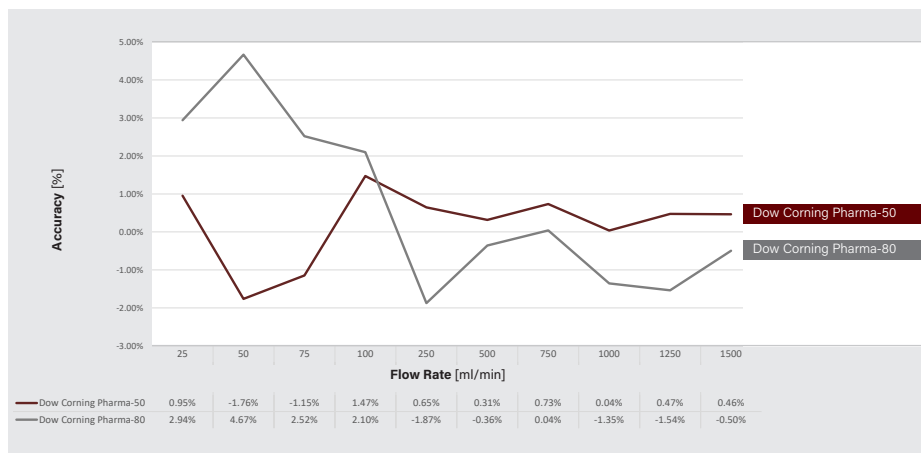

**CONCLUSION:** It is important to adjust the SONOFLOW® sensor when changing the tubing durometer.

Advantapure and Advantasil are trademarks of NewAge Industries, Inc.  
 Dow Corning is a registered trademark of Dow Corning Corporation  
 Cflex, Pharmapure, Tygon are registered trademarks of Saint Gobain Performance Plastics

Sonotec reserves the right to change technical specifications without further notice (Rev. 1 2020-04-01).



3265 Sunset Lane Hatboro, PA 19040 | 215-675-5700 | sentinelprocess.com